

**UNITED STATES AIR FORCE  
RESEARCH LABORATORY**

---



**Measurement of Quantitative IR  
Properties of Single Aerosol  
Particles with Emphasis  
On Biological and Chemical  
Stimulants**

**Richard K. Chang**

**Department of Applied Physics  
Yale University  
New Haven CT 06520**

**September 2004  
Interim Report - June 2003 – June 2004**

**Approved for Public Release; distribution is unlimited**

Human Effectiveness Directorate  
Biosciences and Protection Division  
Counterproliferation Branch  
E5183 Blackhawk Road  
Aberdeen Proving Ground MD 21010-5424

**BEST AVAILABLE COPY**

**20041206 043**

When US Government drawings, specifications or other data are used for any purpose other than definitely related Government procurement operation, the Government thereby incurs no responsibility nor any obligation whatsoever, and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications or other data, is not to be regarded by implication or otherwise, as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

Please do not request copies of this report from the Air Force Research Laboratory.  
Additional copies may be purchased from:

National Technical Information Service  
5285 Port Royal Road  
Springfield, Virginia 22161

Federal Government agencies registered with the Defense Technical Information Center should direct requests for copies of this report to:

Defense Technical Information Center  
8725 John J. Kingman Rd., Ste 0944  
Ft. Belvoir, Virginia 22060-6218

#### TECHNICAL REVIEW AND APPROVAL

AFRL-HE-WP-TR-2004-0121

This report has been reviewed by the Office of Public Affairs (PA) and is releasable to the National Technical Information Service (NTIS). At NTIS, it will be available to the general public, including foreign nations.

This technical report has been reviewed and is approved for publication.

FOR THE DIRECTOR

//signed//

STEPHEN R. CHANNEL, DR-IV  
Director, AF CBD Tech Base Programs  
Air Force Research Laboratory

REPORT DOCUMENTATION PAGE			Form Approved OMB No. 0704-0188	
Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.				
1. AGENCY USE ONLY (Leave blank)		REPORT DATE 1 September 2004	3. REPORT TYPE AND DATES COVERED Interim Report, June 2003 - June 2004	
4. TITLE AND SUBTITLE Measurement of Quantitative IR Properties of Single Aerosol Particles with Emphasis on Biological and Chemical Stimulants			5. FUNDING NUMBERS Contract: F33615-02-2-6066 PE 602384BP PR 1710 TA 1710D6 WU 1710D608	
6. AUTHOR(S) Richard K. Chang				
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) Department of Applied Physics Yale University New Haven CT 06520			8. PERFORMING ORGANIZATION REPORT NUMBER	
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES) Air Force Research Laboratory, Human Effectiveness Directorate, Biosciences and Protection Division, Counterproliferation Branch E5183 Blackhawk Road Aberdeen Proving Ground MD 21010-5424			10. SPONSORING/MONITORING AGENCY REPORT NUMBER  AFRL-HE-WP-TR-2004-0121	
11. SUPPLEMENTARY NOTES				
12a. DISTRIBUTION AVAILABILITY STATEMENT Approved for Public Release; distribution is unlimited.			12b. DISTRIBUTION CODE	
13. ABSTRACT (Maximum 200 words) A simplified experiment in the visible range using 2 wavelengths (one in the absorption band and the other outside the absorption band) was performed initially. We then shifted to the mid-IR (3.41 $\mu\text{m}$ ) using a mixture of $\text{H}_2\text{O}$ and $\text{D}_2\text{O}$ , with the latter being the absorber. Again the peak-to-valley ratio increased upon the addition of $\text{D}_2\text{O}$ into $\text{H}_2\text{O}$ . The angular distribution was collected on the backward scattering direction using an ellipsoidal mirror. The scattered light angle spanned from $0^\circ \leq \theta \leq 360^\circ$ and $90^\circ \leq \theta \leq 163^\circ$ .				
14. SUBJECT TERMS Biological; Biological Defense; Biological Warfare; CBW; Chemical/Biological Defense			15. NUMBER OF PAGES 12	
			16. PRICE CODE	
17. SECURITY CLASSIFICATION OF REPORT Unclassified	18. SECURITY CLASSIFICATION OF THIS PAGE Unclassified	19. SECURITY CLASSIFICATION OF ABSTRACT Unclassified	20. LIMITATION OF ABSTRACT SAR	

THIS PAGE INTENTIONALLY LEFT BLANK

## **Measurement of Quantitative IR Properties of Single Aerosol Particles with Emphasis on Biological and Chemical Stimulants**

*June 2003 to June 2004*

### **Research Participants:**

From Yale – Kevin Aptowicz, Yong-Le Pan, and Richard K. Chang  
From ARL – Ron Pinnick, Steve Hill, Kris Gurton, and Richard Tober  
From Lincoln Labs – Anish Goyal and Tom Jeys  
From AFRL – Burt Bronk

Elastic light scattering is being investigated as a means to extract single particle absorption. In particular, the technique labeled TAOS (Two-dimensional Angular Optical Scattering) detects the angularly resolved elastically scattered light from a particle. These TAOS patterns are sensitive to a particle's morphology (size, shape, structure, and complex refractive index) and therefore can be used to extract information on particle absorption.

Previous work has been done in the visible (532 nm), where the TAOS patterns were successfully shown to vary considerable when the absorptivity of a droplet varied. This matched expectations drawn from Mie theory. The next step was to move the excitation wavelength into the mid-IR where strong absorption bands exist due to molecular vibrational modes.

Two separate experiments were conducted. The first utilizes a lens in the Abbé sine condition to detect the TAOS pattern of single droplets. These TAOS patterns are then compared to Mie theory predictions to deduce the imaginary index from the best-fit. A second experiment was conducted where TAOS patterns at two different wavelengths were simultaneously detected from a single aerosol particle. This dual TAOS patterns were collected over a large solid angle encompassing almost the entire back hemisphere of scattered light. Both systems detect the scattered light in-situ and in real-time.

A simplified schematic of the first experimental arrangement to extract the imaginary part of the refractive index of a spherical particle is shown in figure 1. A liquid dispenser system based on piezo technology generated droplets from an exit orifice (41  $\mu\text{m}$  diameter) at a rate of  $\sim 500$  Hz. The droplet diameter varied from 54  $\mu\text{m}$  to 57  $\mu\text{m}$ . The droplets were composed of three different solutions: distilled water ( $\text{H}_2\text{O}$ ), deuterium oxide ( $\text{D}_2\text{O}$ ), and a 50%-50% mixture of  $\text{H}_2\text{O}$  and  $\text{D}_2\text{O}$ .

The laser source was a type-II InAs/GaInSb interband cascade laser operating in CW mode to generate light at a wavelength of 3.41  $\mu\text{m}$  with optical powers approaching 40 milliwatts. An  $f/2$   $\text{CaF}_2$  plano-convex lens collimated the scattered light onto the detecting focal plane array. The angular range of collected light spanned  $23^\circ$  from  $\theta = 23.5^\circ$  to  $\theta = 46.5^\circ$ . However, because of severe spherical aberration in the outer limits of the angular range the practical collection range was  $26^\circ$  to  $42^\circ$ . These effects were

mitigated by performing an exact ray-trace on the system calculated in Matlab®. The detector, an InSb 320x256 focal-plane-array, was run at a frame rate of 63.13 Hz with an integration window of 217  $\mu$ s so that only a single scattering event would be detected. Three TAOS patterns from the three different solutions are shown in Figure 2. The effects of spherical aberration can be noted by the increase in intensity around the perimeter of the TAOS pattern. Also, the TAOS patterns have different overall signal intensities due to both the effects of particle absorption as well as fluctuations in laser intensity and detected background noise. Thus the data does not lend itself to making an absolute comparison of intensity between data sets.

A cross-section of the TAOS pattern is plotted to the right of each image. The experimental data shows a good match with numerical data based upon Mie theory, although again the effects of spherical aberration can be seen at the edges of the plotted angular range. The input parameters to calculate the Mie theory curve were both experimental measured, as was the case for the droplet diameter, and taken from literature, as was the case of for the complex refractive index. The table below summarizes the input parameters for the different solutions. To calculate the refractive index of H<sub>2</sub>O-D<sub>2</sub>O an average was taken of the H<sub>2</sub>O data and D<sub>2</sub>O data. As one final note, due to variability in particle location, a precise value for the collection angle can not be known. Therefore, overall angle range was slightly shifted ( $\sim 1^\circ$ ) from the measured values to fit the data to theory.

Solution	Complex Refractive Index (at 3.41 $\mu$ m)	Droplet Diameter ( $\mu$ m)
D <sub>2</sub> O	1.279 + i 0.0021	55.176
H <sub>2</sub> O + D <sub>2</sub> O	1.342 + i 0.0098	54.254
H <sub>2</sub> O	1.405 + i 0.0176	57.401

Table 1: Mie theory input parameters

A computer program was written in hopes of extracting the particle's absorptive properties from the raw data. However, due to the noise level, spherical aberration distortions, as well as uncertainty in the angle, the computer analysis was unable to find a strong match to the data set. On the other hand, it is believed that with increase in signal-to-noise ratio as well as a better calibration routine for defining the scattering angles, the complex refractive index, and hence the absorption, can be inferred.

The scheme to collect TAOS images at two wavelengths simultaneously is shown in figure 3. The two laser sources were optically pumped GaSb-based semiconductor lasers with type-II InAs/InGaSb quantum well gain regions emitting at 3.9  $\mu$ m and 5.1  $\mu$ m with a peak power of  $\sim 0.4$  watts and pulse duration of 100  $\mu$ s. Both wavelengths are relatively transparent in H<sub>2</sub>O, but D<sub>2</sub>O has relatively high absorption at 3.9  $\mu$ m while being transparent at 5.1  $\mu$ m. Beam shaping optics (spherical and cylindrical lenses) as well as an F/3.75 CaF<sub>2</sub> focusing lens were utilized to achieve a desired spot size of 50  $\mu$ m x 500  $\mu$ m where the major axis is perpendicular to the propagation direction of the droplet. An ellipsoidal mirror collected the backward hemisphere of scattered light ( $0^\circ \leq \phi \leq 360^\circ$ ,  $90^\circ \leq \theta \leq 163^\circ$ ) and focused it through a spatial filter located at the ellipsoid's second

focal point. To reduce aberrations effects, an F/1 ZnSe aspheric lens collimated the scattered light, after which the two wavelengths were separated via a dichroic mirror. Finally, a bi-convex F/1 CaF<sub>2</sub> lens coupled the scattered light onto the InSb detectors. Droplets from three different mixtures of H<sub>2</sub>O-D<sub>2</sub>O were analyzed: 100%-0%, 75%-25%, and 50%-50%. The experimentally collected data, as well as numerical simulations based on Mie theory, are shown in figure 4. Each column from left to right indicates a different H<sub>2</sub>O-D<sub>2</sub>O droplet composition, as labeled. TAOS patterns (row I) collected at 3.9  $\mu$ m show the effects of increasing the concentration of D<sub>2</sub>O that leads to an increase in absorption. These patterns qualitatively match the numerical simulations based on Mie theory (row II). TAOS patterns (row III) are collected simultaneously at 5.1  $\mu$ m from the same single droplets. These patterns also agree with predictions from Mie theory in which there was a slight increase in scattering intensity of the central region. By comparing the data in row I with row III, it is clear that one could distinguish between droplets of pure H<sub>2</sub>O and droplets that contain a considerable amount of D<sub>2</sub>O by comparing the angular scattering patterns.

As was done in the visible, TAOS patterns of dry aggregate particles were also captured as is shown in figure 5. Due to the low pulse energies of the mid-IR laser, it was difficult to analyze the data since the scattered signal was just above the noise level. However, certain features can be noticed such as the quasi-ring shaped scattering patterns for the Tryptophan and Bovine Albumin particles. This contrasts the scattering patterns seen in the visible which are primarily made up of island like features. The reason for these ring-like patterns is the shift in wavelength to a size comparable to the particle diameter. Thus the laser light is no longer sensitive surface roughness of the particle, rather just its overall shape.

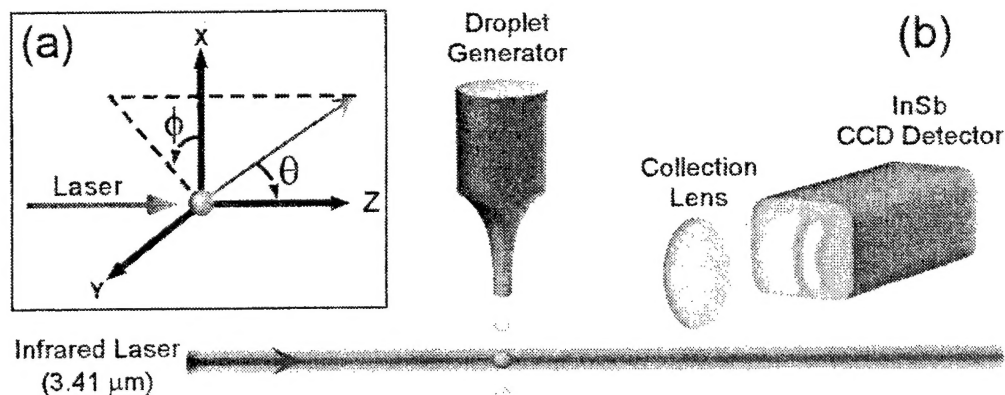


Figure 1: Experimental Set-up

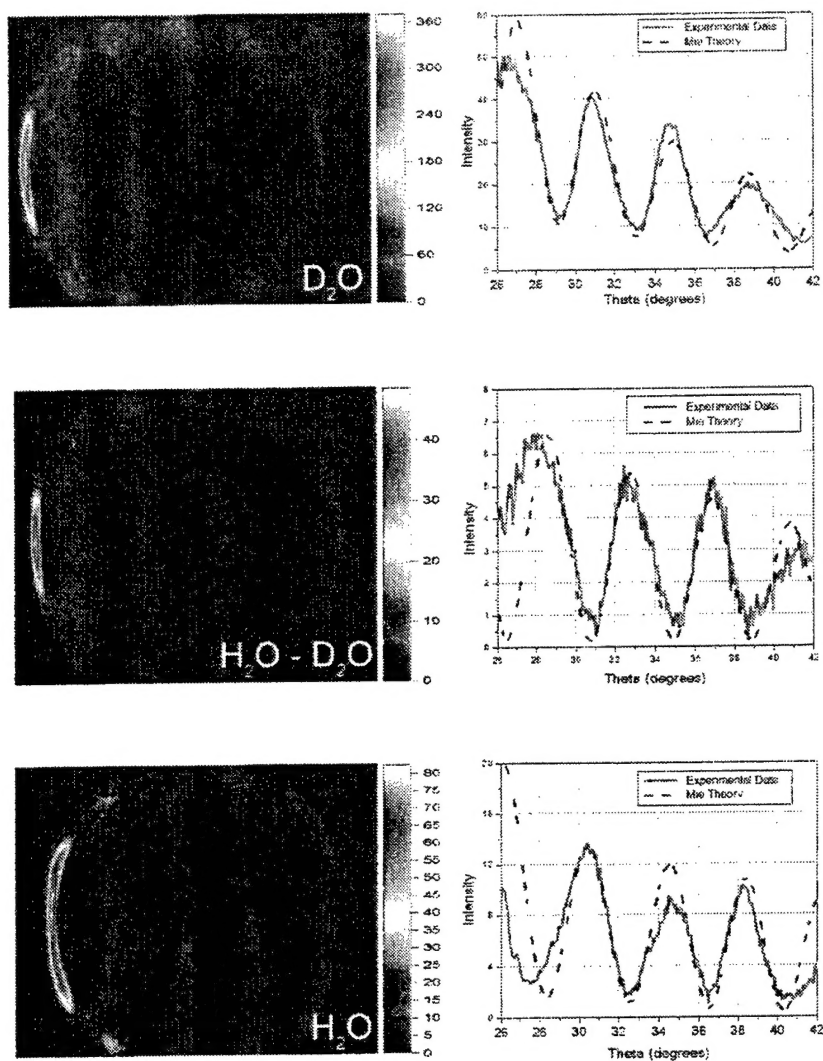


Figure 2: Left, TAOS patterns collected from droplets of  $D_2O$ , 50/50  $H_2O$ - $D_2O$  mixture, and  $H_2O$ . Right, horizontal cross-sections of the TAOS patterns are compared with Mie theory results.



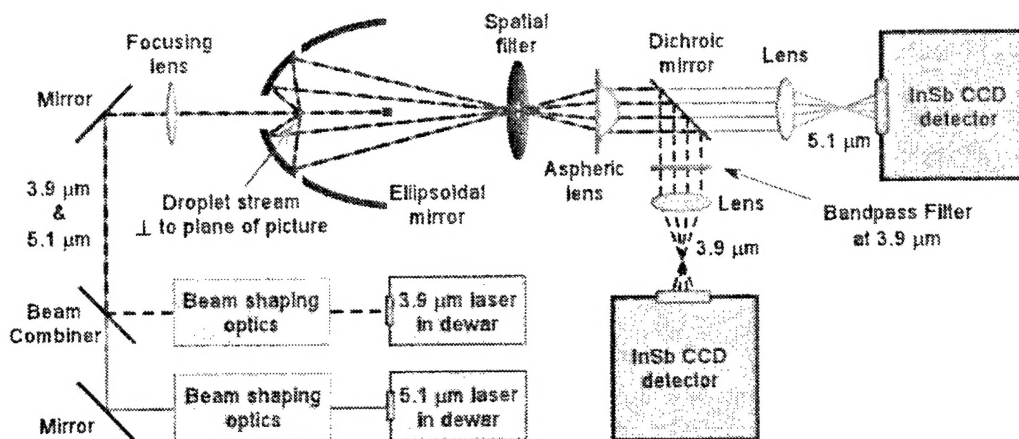


Figure 3: Experimental set-up to collect simultaneous TAOS patterns at two wavelengths.

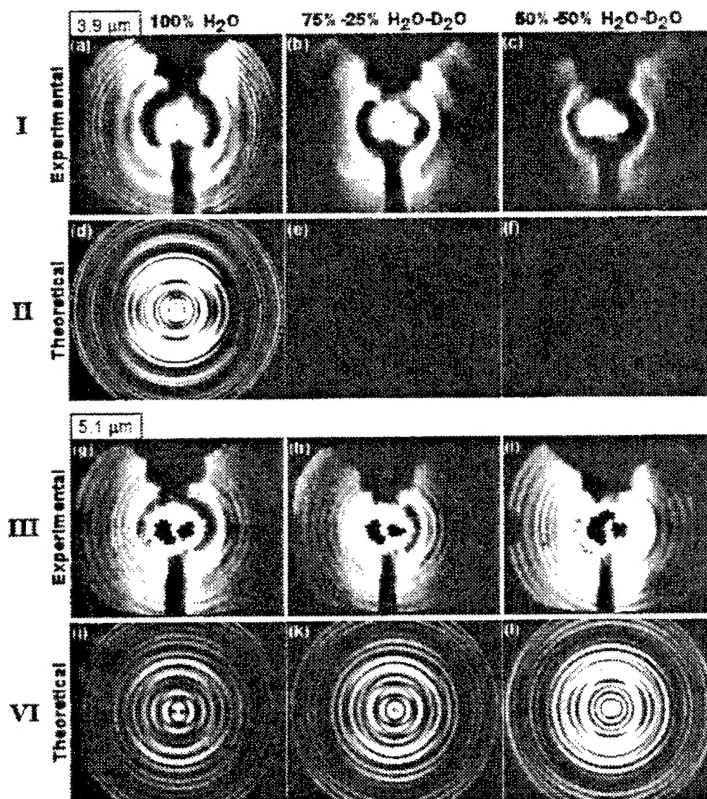


Figure 4: (Row I) TAOS pattern at  $\lambda = 3.9 \mu\text{m}$  detected from a single droplet (diameter  $\sim 55 \mu\text{m}$ ) composed of (a)  $\text{H}_2\text{O}$ , (b) 75%-25%  $\text{H}_2\text{O}-\text{D}_2\text{O}$ , and (c) 50%-50%  $\text{H}_2\text{O}-\text{D}_2\text{O}$ . (Row II) Corresponding numerical simulations of row I based upon Mie theory. (Row III) TAOS pattern collected simultaneously at  $5.1 \mu\text{m}$  from the same single droplets as row I. (Row IV) Corresponding numerical simulations of row III based upon Mie theory.

**Simultaneously Captured  
Dual TAOS patterns of 8  $\mu\text{m}$  aerosols**

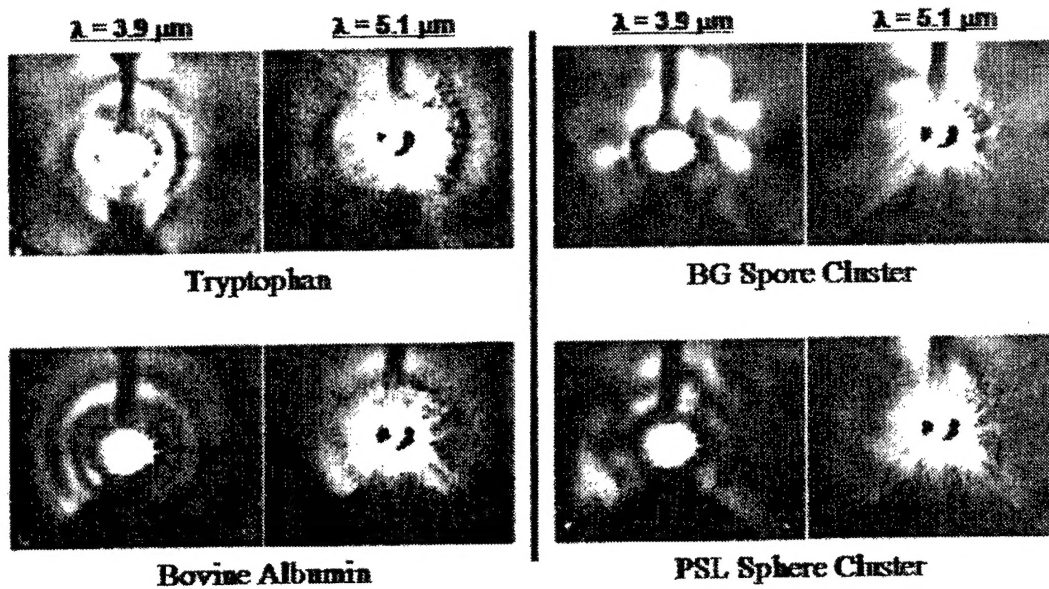


Figure 5: TAOS patterns captured simultaneously of dry aggregate particles.

## PUBLICATIONS

*Two-dimensional angular optical scattering patterns in the mid-infrared of microdroplets: on and off absorption*, K.B. Aptowicz, Y.L. Pan, and R.K. Chang, R.G. Pinnick, S.C. Hill, R.L. Tober, B.V. Bronk, to be published in September issue of Optics Letters.

*Characterizing and monitoring respiratory aerosols by light scattering*, Y.L. Pan, K.B. Aptowicz, R.K. Chang, M. Hart, and J.D. Eversole, Optics Letters, 28 (8), 589-591, (2003).

## CONFERENCE PAPERS AND TALKS GIVEN BY KEVIN APTOWICZ

*Elastic light scattering and laser-induced fluorescence, optical techniques for bio-aerosol enrichment*, K.B. Aptowicz and R.K. Chang, Seminar Talk at Sandia National Labs (2004).

*Two-dimensional angular optical scattering (TAOS) of single aerosol particles in the visible and mid-infrared*, K.B. Aptowicz, Y.L. Pan, and R.K. Chang, 2004 Scientific Conference on Obscuration and Aerosol Research.

*Large angle two-dimensional angular optical scattering (LA TAOS) in the mid-infrared of single aerosol particles*, K.B. Aptowicz, Y.L. Pan, R.K. Chang, and B.V. Bronk, 2<sup>nd</sup> Joint Conference on Point Detection for Chemical and Biological Defense (2004).

*Two-dimensional angular optical scattering patterns in the mid-infrared of microdroplets: on and off absorption*, K.B. Aptowicz, Y.L. Pan, R.K. Chang, R.G. Pinnick, S.C. Hill, K. Gurton, R.L. Tober, and B.V. Bronk, 2003 Joint Service Scientific Conference on Chemical & Biological Defense Research.

*Two-dimensional angular optical scattering patterns of aerosol particles in the mid-infrared: measurements designed to obtain particle absorption*, K.B. Aptowicz, Y.L. Pan, R. K. Chang, R.G. Pinnick, S.C. Hill, K. Gurton, R.L. Tober, and B.V. Bronk, 2003 SPIE Photonics East, contributed oral presentation and paper.

*Distinguishing aerosol features via elastic scattering: absorption, inclusion, and colloid*, K. B. Aptowicz, K.B. Aptowicz, Y.L. Pan, M. Surbek, R.K. Chang, 2003 Conference on Lasers and Electro Optics (CLEO).

*Efficient light collection for a low-cost respiratory oxygen sensor*, K.B. Aptowicz and R. Hooker, Proceedings of SPIE vol. 4446, pages 221-231, 2001 SPIE Annual Meeting, contributed oral presentation and paper.

CONFERENCE PAPERS AND TALKS GIVEN  
BY RICHARD K. CHANG

University of Milan, Sept 4, 2003, Milan, Italy

Optical Society of America Annual Meeting, Oct 6-10, 2003  
Tuscon, AZ

SUVOS-Darpa-Progress Report Meeting, Nov 18-19, Austin,  
TX

Fudan University, May 11, 2004, Shanghai, China

Hong Kong University of Science and Technology, May 17,  
2004, Hong Kong, China